



Sleep Fairy-A9

- ✓ Good user experience, comfortable to wear
- ✓ Real-time display of each waveform data, clear to view
- ✓ Patent chest and abdomen signal acquisition, easy to use
- ✓ Rechargeable battery, environmental protection
- ✓ High-speed SD storage card, more durable



Required Departments

Pneumology
Department

E.N.T
Department

Neurology

Geriatric
Department

Cardiology
Department


Endocrinology
Department

Pediatrics
Department

--- Features ---

✓ Advanced high-precision 3D gyroscope technology

Acquire users' chest and abdomen breathing effect according to 3D gyroscope technology, which do not affect by patients' body position, strong anti-interfere performance and high sensitivity.

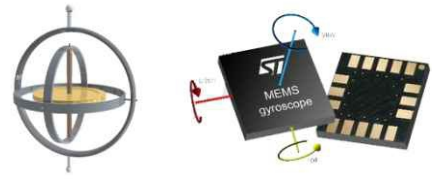

✓ Smart appearance, only 176g with battery

✓ 9 Parameters: SpO2, Pulse, Pulse Waveform, Airflow, Snoring, Chest/Abdomen Movement, Body Position, Body Movement, CPAP Pressure

✓ Patented chest & abdomen signal acquisition

Greatly reduce workload and use cost, more effective and portable.

✓ Easy to use


Quick to learn, high reliability, low maintenance cost.

✓ High speed SD card for data record without computer operation system limited

Easy to extend storage space, supports Windows XP/ 7/ 8/ 10 and 32/64 bit system.

✓ Large capacity rechargeable lithium battery

Economic and environmental, supportable for 30 hours continuously monitoring (over 4 nights).

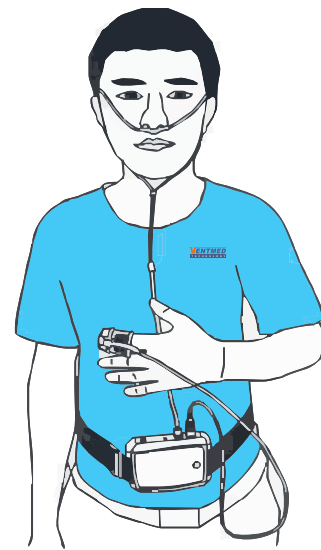

Wearing Sketch



✓ 2.8" color screen

Real time display of all waveform data, intuitive and efficient.


✓ Intelligent analysis software

Automatically analyze all kinds of breathing events and accuracy is above 95%, very useful for doctors and other related people (coach and nurses etc).


✓ Friendly interface, nice UI graphic design, support for Windows XP/ 7/ 8/ 10 operation system.

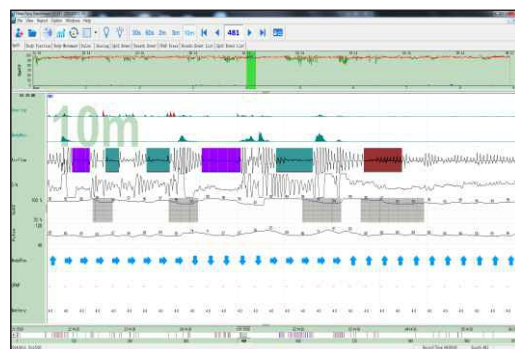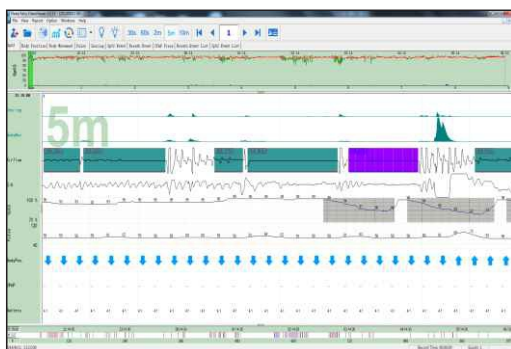


- ✔ Multiple sleep monitor reports, facilitate physician know patient's condition, and formulate a reasonable therapeutic schedule

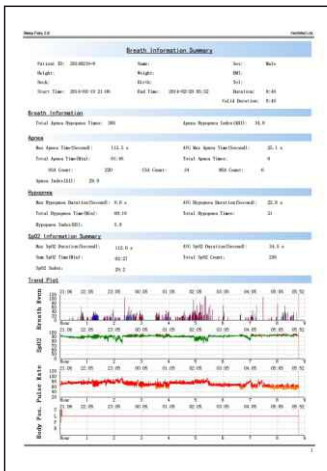

Breath Information Summary

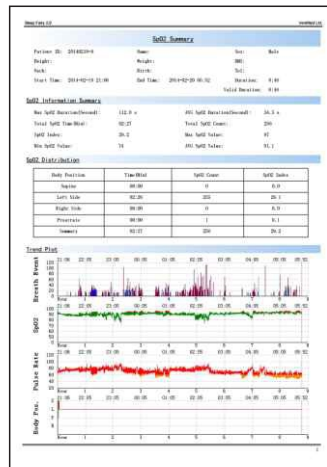


SpO2 Summary

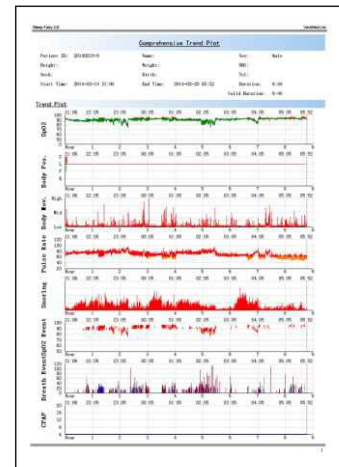

Comprehensive Trend Plot




Sleep Monitor Report

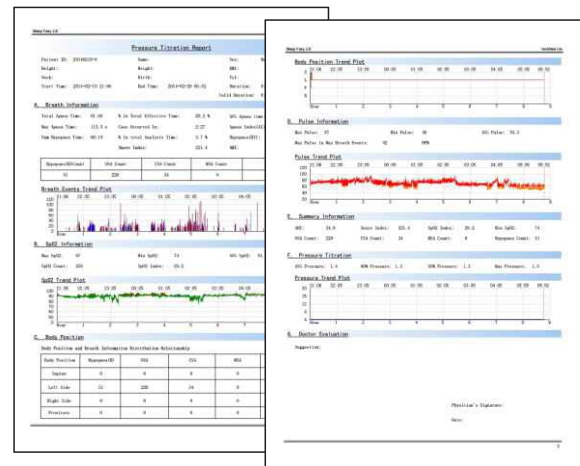

Pressure Titration Report

- Multiple report templates, support WORD/PDF format and customization.
- Convenient user data management.
- Original data pages to print.

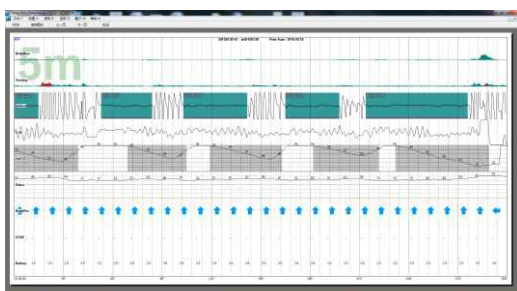

Patient Information

Patient Information | Data Information

Patient ID: 20140811-10 Start Time: 2014-08-11 21:15 End Time: 2014-08-12 00:10 Duration: 00:55:30

17171000-Recor-ID

Person Information

Name: Sex: ☐ G 1-Male / 2-Female

Birthdate: 1902/ 5/24 Age: 0

Weight: 0.00 kg Height: 0.00 cm

BMI: 0.00 Neck: 0.00 cm

Tel: E_mail:

Addr:

Comment:

Save to: C:\Data Files\20140811-10\

OK Close

[illegible]

Specification

Description	Sleep Fairy-A9
9 Parameters	Airflow, Snoring, SpO2, Chest/Abdomen Movement, Pulse, Pulse Waveform, Body Movement, Body Position, CPAP Pressure
Data Resolution	AD : 12Bit
Data Sampling Rate	50-200Hz
Storage Date	16G, over 16000 hours data
Communication	SD card
SpO2	70% - 100%
Pulse	30 - 240 bpm
Battery	Integrated Rechargeable Lithium Battery, 2500 mAh
Continuous Recording Time	30 hours
Screen	2.8 inch TFT, 320 x 240
Device Net Weight	176g with battery
Gross Weight	0.9Kg
Device Dimensions	125mmL x 80mmW x 24mmH
Carton Size	385mmL x 365W x 160mmH



Tel: +27 10 211 9136
 Mobile: +27 63 231 4269
 E-Mail: cbmadmin@iafrica.com
www.cbmmmedical.co.za
 Reg No.:2009/0179685/07
 Practice No: 0972274
 VAT: 4390254060